




Mass Spectrometry Report

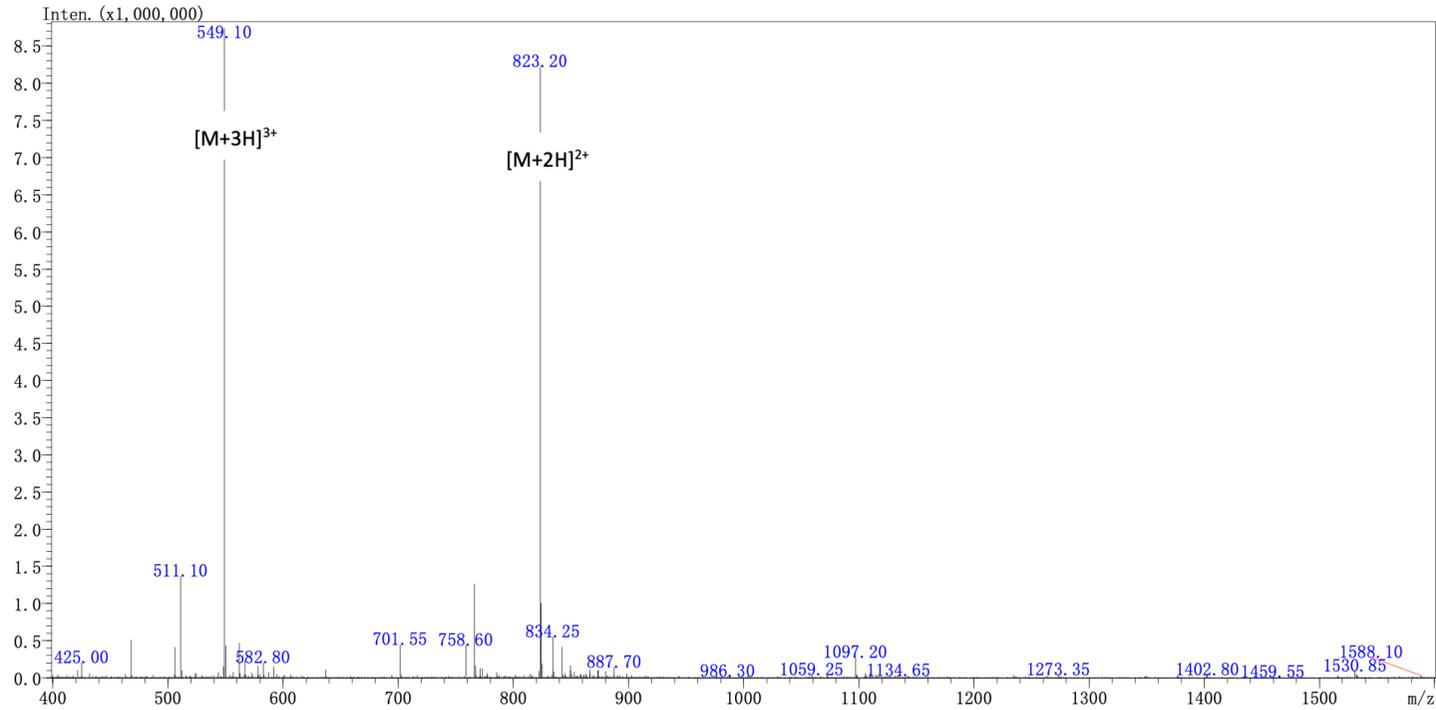

Sample Description

Analyzed date: 20250418,14:19

Analyst: KWX

Sample: KP3964-5

M.W.: 1644.77

Lot. No.: 20250416

Instrument SHIMADZU LCMS-2020

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250°C

Block Temp.: 200°C

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 0.05%FA in 30%H₂O/30%ACN/40%MeOH